


# Wondfo®



**+** NEW POCT SOLUTION



**PRODUCT CATALOG | 2018**



## WONDFO PROFILE **Stock Code: 300482**

Guangzhou Wondfo Biotech Co., Ltd., located in Guangzhou, China, is a globally recognized fast growing POCT company devoted to the R&D, manufacture and sales of rapid diagnostic reagents and related equipment in IVD (*in vitro* diagnostic) field.

Founded in 1992, the company is continually expanding its scale. Apart from the Guangzhou headquarters, Wondfo also owns one overseas R&D center in San Diego, one branch in Chicago and more than ten overseas offices. Wondfo went public in June, 2015 (Stock Code: 300482), and has more than 1,500 employees.

As one of the earliest high-tech biological companies focusing on rapid diagnostics for toxicology, infectious diseases, fertility, cardiovascular disease, tumor, respiratory disease, renal injury and diabetes. Wondfo has won good reputation around the world. In addition, Wondfo has got CE certificates, FDA certificates, FSC certificates, ISO 9001:2015 and ISO 13485:2016 quality system certification.

We are dedicated to making the world a better place by providing people with high quality products and services.



## 01 Professional R&D Team

Wondfo has been consistently paying attention to R&D and regarding innovation as the core of its development. As a result, there are highly educated employees in the company. And it owns well-equipped research laboratories in both Guangzhou (covering nearly 5,000 square meters) and San Diego, USA.

## 02 Strong Production Capacity

With the international leading production lines and highly experienced staff, its daily production capacity reaches to 1.5 million test strips. Services are also tailored to professional distributors and partnering affiliates.

## 03 Integrated Services System

Covering more than 180 countries and areas, Wondfo provides an exciting opportunity to distribute quality products at very competitive price. Every aspect of the company's operation is strictly measured, which provides customers with all-around technical support and counselling all the time.

# Focus on *POCT* Industry




## Applications



# CERTIFICATES



ISO 13485



ISO9001



CE



FDA



Guangzhou Wondfo Biotech Co., Ltd.

# CONTENTS

## Qualitative Rapid Diagnostic Family

### Fertility Tests

02

hCG Pregnancy Test  
Sperm Concentration Test  
LH Ovulation Test  
FSH Urine Test

### Infectious Disease Tests

03-04

HBsAg Hepatitis B Surface Antigen Test  
HBV Hepatitis B Virus Test  
HBsAb Hepatitis B Surface Antibody Test  
HCV Hepatitis C Virus Test  
HIV 1/2 Blood Test (2 Lines)  
HIV 1/2 Blood Test (3 Lines)  
HIV 1/2 Oral Mucosal Transudate Test  
Malaria P.f Test  
Malaria P.f/Pan Test  
Malaria P.f/P.v Test  
H.Pylori Test  
Flu A Test  
Flu B Test  
Flu A&B Tset  
Dengue NS1 Antigen Test  
Dengue IgG/IgM Antibody Test  
Combined Dengue NS1 Antigen and Dengue IgG/IgM Antibody Test  
Adenovirus Test  
Rotavirus Test  
Combined Adenovirus and Rotavirus Test  
MP Mycoplasma pneumonia Test  
H7 Subtype Influenza Test  
HAV Hepatitis A Virus Test  
HEV Hepatitis E Virus Test  
HIV-HCV-HBsAg-Syphilis Test  
HIV-HCV-HBsAg-HBsAb-Syphilis Test  
HIV-HCV-HBsAg-HBcAb-Syphilis Test  
Strep A Test  
CP Chlamydia Pneumoniae Test  
Enterovirus 71 Test  
Syphilis Test  
Chlamydia Test  
Gonorrhea Test

### Tumor Marker Tests

04

FOB Fecal Occult Blood Test  
PSA Prostate Specific Antigen Test

### Cardiac Marker Tests

04

Troponin I Test  
H-FABP Test

### Drug of Abuse Tests (Urine)

04-07

Multi-Test Panel  
Multi-Test T-Cup  
Multi-Test Q-Cup  
Multi-Test K-Cup  
AMP Amphetamine Test  
BAR Barbiturates Test  
CAF Caffeine Test  
BZO Benzodiazepines Test  
COC Cocaine Test  
MET Methamphetamine Test  
MDMA Test  
BUP Buprenorphine Test  
MOP Morphine Test  
MTD Methadone Test  
OPI Opiate Test  
PCP Phencyclidine Test  
TCA Tricyclic Antidepressants Test  
THC Marijuana Test  
OXY Oxycodone Test  
KET Ketamine Test  
PPX Propoxyphene Test  
EDDP Test  
TRA Tramadol Test  
K2 Synthesis Cannabis Test  
FTY Fentanyl Test  
COT Cotinine Test  
ETG Ethylglucuronide Test  
MQL Methaqualone Test  
MC Methcathinone Test  
Alcohol Saliva Test

### Drug of Abuse Test (Oral fluid)

07

Multi-Drug 6 Test  
Multi-Drug T-Cube

### DOA Reader

07

Handheld Colloidal Gold Test Analyzer  
Multi-Drug Panel for Analyzer

### Other Rapid Tests

07

Urinalysis Reagents Strip

## Quantitative Detection Family

08-11

### Blood Gas Analyzer

09

### Optical Coagulation Analyzer

10

### Blood Glucose Monitoring System

11

### Immunofluorescence Quantitative Test System

11



## Qualitative Rapid Diagnostic Family

- Infectious Disease Tests
- Tumor Marker Tests
- Alcohol Tests
- Cardiac Tests
- Urinalysis Reagents Strip



### • Fertility Tests



Pregnancy & Ovulation tests

▼ DM-102 (Disposable)



▼ DM-111 (Reusable)




Digital Pregnancy Test

▼ DLH-101 (Reusable)



Digital Ovulation Test



Sperm Concentration Test Kit

### • DOA Urine Tests



Cassette



Strip



Panel



Q-Cup

T-Cup

Key-Cup

### • DOA Urine Tests

























### • DOA Oral Fluid Tests




DOA Oral Fluid Tests



## Fertility Test: Pregnancy Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W1-S	hCG Pregnancy Test	Strip	3.0/3.5/4.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-S1H2
W1-C	hCG Pregnancy Test	Cassette	4.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-C1H2
W1-C1	hCG Pregnancy Test	Cassette I	3.5 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-CI1H2
W1-M	hCG Pregnancy Test	Midstream	6.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-M1H2
W1-M II	hCG Pregnancy Test	Midstream II	5.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-MII1H2
W1-M III	hCG Pregnancy Test	Midstream III	6.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-MIII1H2
W1-M4	hCG Pregnancy Test	Midstream 4	3.5 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-M41H2
W1-M6	hCG Pregnancy Test	Midstream 6	6.0 mm	Urine	25/10 mIU/mL	 FDA CLIA	W001-M61H2
W1-S3 P	hCG Pregnancy Test	Strip	3.0/3.5 mm	Serum/Urine	25 mIU/mL	 FDA CLIA	W001-S3P2
W1-C3 P	hCG Pregnancy Test	Cassette	4.0 mm	Serum/Urine	25 mIU/mL	 FDA CLIA	W001-C3P2
W1-S(20mIU)	hCG Pregnancy Test	Strip	3.0/3.5/4.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-S1H202
W1-C(20mIU)	hCG Pregnancy Test	Cassette	4.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-C1H202
W1-C1(20mIU)	hCG Pregnancy Test	Cassette I	3.5 mm	Urine	20 mIU/mL	 FDA CLIA	W001-CI1H202
W1-M(20mIU)	hCG Pregnancy Test	Midstream	6.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-M1H202
W1-M II(20mIU)	hCG Pregnancy Test	Midstream II	5.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-MII1H202
W1-M III(20mIU)	hCG Pregnancy Test	Midstream III	6.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-MIII1H202
W1-M4(20mIU)	hCG Pregnancy Test	Midstream 4	3.5 mm	Urine	20 mIU/mL	 FDA CLIA	W001-M41H202
W1-M6(20mIU)	hCG Pregnancy Test	Midstream 6	6.0 mm	Urine	20 mIU/mL	 FDA CLIA	W001-M61H202
DM-102	Digital Pregnancy Test (Disposable)	Midstream	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W941-M1H102
DM-111	Digital Pregnancy Test (Reuseable)	Midstream	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W941-M1H102
W121-S	Sperm Concentration Test	Strip	3.0/3.5/4.0 mm	Semen	15x10 <sup>6</sup> /mL	 FDA CLIA	W121-S0H102
W121-C	Sperm Concentration Test	Cassette	4.0 mm	Semen	15x10 <sup>6</sup> /mL	 FDA CLIA	W121-C0H102

## Fertility Tests: Ovulation Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W2-S	LH Ovulation Test	Strip	3.0/3.5/4.0 mm	Urine	25 mIU/mL	 FDA CLIA	W002-S1H2
W2-C	LH Ovulation Test	Cassette	4.0 mm	Urine	25 mIU/mL	 FDA CLIA	W002-C1H2
W2-C I	LH Ovulation Test	Cassette I	3.5 mm	Urine	25 mIU/mL	 FDA CLIA	W002-CI1H2
W2-M	LH Ovulation Test	Midstream	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W002-M1H2
W2-M II	LH Ovulation Test	Midstream II	5.0 mm	Urine	25 mIU/mL	 FDA CLIA	W002-MII1H2
W2-M4	LH Ovulation Test	Midstream 4	3.5 mm	Urine	25 mIU/mL	 FDA CLIA	W002-M41H2
W2-M6	LH Ovulation Test	Midstream 6	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W002-M61H2
DLH-101	Digital Ovulation Test (Reuseable)	Midstream	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W941-M1H101
W52-S	FSH Urine Test	Strip	3.0/3.5/4.0 mm	Urine	25 mIU/mL	 FDA CLIA	W052-S1H2
W52-C	FSH Urine Test	Cassette	4.0 mm	Urine	25 mIU/mL	 FDA CLIA	W052-C1H2
W52-M	FSH Urine T est	Midstream	6.0 mm	Urine	25 mIU/mL	 FDA CLIA	W052-M1H2

## Infectious Disease Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W003-S	HBsAg	Strip	2.5/3.0 mm	Serum/Plasma/Whole Blood	2 ng/mL		W003-S4P2
W003-C	HBsAg	Cassette	4.0 mm	Serum/Plasma/Whole Blood	2 ng/mL		W003-C4P2
W040-P	HBV	Panel	4.0 mm	Serum/Plasma/Whole Blood	/		W040-P4P2
W004-S	HBsAb	Strip	2.5/3.0 mm	Serum/Plasma/Whole Blood	/		W004-S2P2
W004-C	HBsAb	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W004-C2P2
W005-S	HCV	Strip	4.0 mm	Serum/Plasma/Whole Blood	/		W005-S4P2
W005-C	HCV	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W005-C4P2
W006-C4P2	HIV 1/2(2 Lines)	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W006-C4P2
W050-C	HIV 1/2 (3 Lines)	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W050-C4P2
W063-S	HIV 1/2 Oral Mucosal Transudate Test	Strip	4.0 mm	Oral Mucosal Transudate	/		W063-S9P2
W063-C	HIV 1/2 Oral Mucosal Transudate Test	Cassette	4.0 mm	Oral Mucosal Transudate	/		W063-C9P2
W37-S	Malaria P.f	Strip	2.5/3.0 mm	Whole Blood	/	CE	W037-S7P2
W37-C	Malaria P.f	Cassette	4.0 mm	Whole Blood	/	CE	W037-C7P2
W62-C	Malaria P.f/Pan	Cassette	4.0 mm	Whole Blood	/	CE	W062-C7P2
W056-C	Malaria P.f/P.v	Cassette	4.0 mm	Whole Blood	/	CE	W056-C7P2
W38-S	H.Pylori Antibody Test	Strip	2.5/3.0 mm	Serum/Plasma	/	CE	W038-S2P2
W38-C	H.Pylori Antibody Test	Cassette	4.0 mm	Serum/Plasma	/	CE	W038-C2P2
W028-C	H.Pylori Antigen Test	Cassette	4.0 mm	Feces	/	CE	W028-C6P2
W71-C	Flu A&B	Cassette	4.0 mm	Nasal Swab	Flu A: 5.1x10 <sup>5</sup> TCID <sub>50</sub> /mL Flu B: 1.5x10 <sup>6</sup> TCID <sub>50</sub> /mL	CE 0123	W059-C0P2
W72-C	Flu A	Cassette	4.0 mm	Nasal Swab	Flu A: 5.1x10 <sup>5</sup> TCID <sub>50</sub> /mL	CE 0123	W060-C0P2
W73-C	Flu B	Cassette	4.0 mm	Nasal Swab	Flu B: 1.5x10 <sup>6</sup> TCID <sub>50</sub> /mL	CE 0123	W061-C0P2
W041-C	Dengue NS1 Antigen Test	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W041-C4P2
W109-C	Dengue IgG/IgM Antibody Test	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W034-S4P3
W111-C	Combined Dengue NS1 Antigen and IgG/IgM Antibody Test	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W034-C4P3
W112-C	Rotavirus	Cassette	3.0 mm	Feces	/	CE	W035-C5P2
W133-C	Adenovirus	Cassette	3.0 mm	Feces	/	CE	W036-S5P2
W134-C	Combined Rotavirus Antigen and Adenovirus Antigen Test	Cassette	3.0 mm	Feces	/	CE	W036-C5P2
W113-C	MP Mycoplasma Pneumonia	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W046-C4P2
W108-C	H7 Subtype Influenza	Cassette	2.5 mm	Sputum/Swab	1 ng/mL		W020-C4G1
W071-C	HAV	Cassette	4.0 mm	Serum/Plasma	/	CE	W109-C4P3
W072-C	HEV	Cassette	4.0 mm	Serum/Plasma	/	CE	W111-C4P4
W026-C	HIV-HCV-HBsAg-Syphilis	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W112-C6P2
W027-C	HIV-HCV-HBsAg-HBsAb-Syphilis	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W133-C6P2
W61-P	HIV-HCV-HBsAg-HBcAb-Syphilis	Cassette	4.0 mm	Serum/Plasma/Whole Blood	/		W134-C6P2
W39-S	Strep A	Strip	2.5/3.0 mm	Swab	/	CE FDA	W113-C4P3
W39-C	Strep A	Cassette	4.0 mm	Swab	/	CE FDA	W108-C9P2
W135-C	Chlamydia Pneumoniae	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE 0123	W071-C4P2
W141-S	Enterovirus 71	Strip	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W072-C4P2
W141-C	Enterovirus 71	Cassette	3.0 mm	Serum/Plasma/Whole Blood	/	CE	W026-C4P2
W34-S4P	Syphilis	Strip	2.5/3.0 mm	Serum/Plasma/Whole Blood	/	CE	W027-C4P2

## Infectious Disease Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W34-C4P	Syphilis	Cassette	4.0 mm	Serum/Plasma/Whole Blood		CE	W027-P4P2
W35-C	Chlamydia	Cassette	4.0 mm	Swab/Urine	/	CE <sub>0123</sub>	W039-S5P2
W36-S	Gonorrhea	Strip	2.5/3.0 mm	Swab	/	CE	W039-C5P2
W36-C	Gonorrhea	Cassette	4.0 mm	Swab	/	CE	W135-C4P2

## Tumor Marker Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W030-S	FOB	Strip	2.5/3.0 mm	Feces	50 ng/mL	CE <sub>0123</sub>	W030-S6P502
W030-C	FOB	Cassette	4.0 mm	Feces	50 ng/mL	CE <sub>0123</sub> FDA CLIA	W030-C6P502
W30-S	FOB	Strip	2.5/3.0 mm	Feces	200 ng/mL	CE	W030-S6P2002
W30-C	FOB	Cassette	4.0 mm	Feces	200 ng/mL	CE	W030-C6P2002
W31-S	PSA	Strip	2.5/3.0 mm	Serum/Plasma	4 ng/mL	CE <sub>0123</sub>	W031-S2P2
W31-C	PSA	Cassette	4.0 mm	Serum/Plasma	4 ng/mL	CE <sub>0123</sub>	W031-C2P2

## Cardiac Marker Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W46-C4P	Troponin I Test	Cassette	4.0 mm	Serum/Plasma/Whole Blood	1 ng/mL	CE	W046-C4P2
W020	H-FABP Test	Cassette	4.0 mm	Serum/Plasma/Whole Blood	7 ng/mL		W020-C4G1

## Drug of Abuse Tests (Urine)

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W2002~2012-P	Multi-Drug 2~12	Panel	4.0mm	Urine	Variable	CE FDA CLIA	W2002~2012-P1G1
W2013~2016-P	Multi-Drug 13~16	Panel	4.0mm	Urine	Variable	CE	W2013~2016-P1G1
W2002~2010-CU	Multi-Drug 2~10	K-Cup	4.0/3.5mm	Urine	Variable	CE FDA CLIA	W2002~2010-CU1G1
W2011~2012-CU	Multi-Drug 11~12	K-Cup	3.5mm	Urine	Variable	CE FDA CLIA	W2011~2012-CU1G1
W502~518-CU2	Multi-Drug 2~18	T-Cup	2.5mm	Urine	Variable	CE FDA CLIA	W502~518-CU21G1
W502~518-CU3	Multi-Drug 2~18	Q-Cup	2.5 mm	Urine	Variable	CE FDA CLIA	W502~518-CU31G1
W502~518-CU8	Multi-Drug 2~18	T-Cup Plus	2.5mm	Urine	Variable	CE	W502~518-CU81G1
W502~518-CU7	Multi-Drug 2~18	Q-Cup Plus	2.5 mm	Urine	Variable	CE	W502~518-CU71G1
W7-S	AMP (Amphetamine)	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL	CE FDA CLIA	W007-S1G1
					500 ng/mL	CE	W007-S1G5001
					300 ng/mL		W007-S1G3001
W7-C	AMP (Amphetamine)	Cassette	4.0mm	Urine	1000 ng/mL	CE FDA CLIA	W007-C1G1
					500 ng/mL	CE	W007-C1G5001
					300 ng/mL		W007-C1G3001
W7-P	AMP (Amphetamine)	Panel	4.0mm	Urine	1000 ng/mL	FDA CLIA	W007-P1G1
					500 ng/mL	CE FDA CLIA	W007-P1G5001
					300 ng/mL	FDA	W007-P1G3001

## Drug of Abuse Tests (Urine)

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W8-S	BAR (Barbiturates)	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL	CE FDA CLIA	W008-S1G1
					200 ng/mL		W008-S1G2001
W8-C	BAR (Barbiturates)	Cassette	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W008-C1G1
					200 ng/mL		W008-C1G2001
W8-P	BAR (Barbiturates)	Panel	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W008-P1G1
					200 ng/mL		W008-P1G2001
W13-S	BUP (Buprenorphine)	Strip	2.5/3.0/3.5/4.0mm	Urine	10 ng/mL	CE FDA	W013-S1G1
W13-C	BUP (Buprenorphine)	Cassette	4.0mm	Urine	10 ng/mL	CE	W013-C1G1
W13-P	BUP (Buprenorphine)	Panel	4.0mm	Urine	10 ng/mL	CE FDA CLIA	W013-P1G1
W9-S	BZO (Benzodiazepines)	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL	CE FDA CLIA	W009-S1G1
					200 ng/mL		W009-S1G2001
					100 ng/mL		W009-S1G1001
W9-C	BZO (Benzodiazepines)	Cassette	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W009-C1G1
					200 ng/mL		W009-C1G2001
					100 ng/mL		W009-C1G1001
W9-P	BZO (Benzodiazepines)	Panel	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W009-P1G1
					200 ng/mL		W009-P1G2001
					100 ng/mL		W009-P1G1001
W083-S	CAF (Caffeine)	Strip	2.5/3.0/3.5/4.0mm	Urine	8 ug/ml		W083-S1G1
W083-C	CAF (Caffeine)	Cassette	4.0mm	Urine	8 ug/ml		W083-C1G1
W083-P	CAF (Caffeine)	Panel	4.0mm	Urine	8 ug/ml		W083-P1G1
W10-S	COC (Cocaine)	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL	CE FDA	W010-S1G1
					150 ng/mL		W010-S1G1501
					100 ng/mL		W010-P1G1
W10-C	COC (Cocaine)	Cassette	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W010-S1G1001
					150 ng/mL		W010-C1G1
					100 ng/mL		W010-C1G1501
W10-P	COC (Cocaine)	Panel	4.0mm	Urine	300 ng/mL	CE FDA CLIA	W010-P1G1
					150 ng/mL		W010-P1G1501
					100 ng/mL		W010-P1G1001
W139-S	COT (Cotinine)	Strip	2.5/3.0/3.5/4.0mm	Urine	100 ng/mL	CE	W139-S1G1
W139-C	COT (Cotinine)	Cassette	4.0mm	Urine	100 ng/mL	CE	W139-C1G1
W139-P	COT (Cotinine)	Panel	4.0mm	Urine	100 ng/mL	CE	W139-P1G1
W074-S	EDDP	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL	CE	W010-S1G1
					100 ng/mL		W010-S1G1001
W074-C	EDDP	Cassette	4.0mm	Urine	300 ng/mL	CE	W010-C1G1
					100 ng/mL		W010-C1G1001
W074-P	EDDP	Panel	4.0mm	Urine	300 ng/mL	CE	W010-P1G1
					100 ng/mL		W010-P1G1001
W140-S	ETG	Strip	2.5/3.0/3.5/4.0mm	Urine	500 ng/mL	CE	W140-S1G1
W140-C	ETG	Cassette	4.0mm	Urine	500 ng/mL	CE	W140-C1G1
W140-P	ETG	Panel	4.0mm	Urine	500 ng/mL	CE	W140-P1G1
W087-S	FTY (Fentanyl)	Strip	2.5/3.0/3.5/4.0mm	Urine	20 ng/mL	CE	W087-S1G1
W087-C	FTY (Fentanyl)	Cassette	4.0mm	Urine	20 ng/mL	CE	W087-C1G1
W087-P	FTY (Fentanyl)	Panel	2.5/3.0/3.5/4.0mm	Urine	20 ng/mL	CE	W087-P1G1
W089-S	K2 (Synthetic Cannabis)	Strip	4.0mm	Urine	JWH-018 Pentanoic Acid: 50 ng/mL, JWH-073 Butanoic Acid: 25 ng/mL	CE	W089-S1G1
W089-C	K2 (Synthetic Cannabis)	Cassette	4.0mm	Urine	JWH-018 Pentanoic Acid: 50 ng/mL, JWH-073 Butanoic Acid: 25 ng/mL	CE	W089-C1G1

## Drug of Abuse Tests (Urine)

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W089-P	K2 (Synthetic Cannabis)	Panel	4.0mm	Urine	JWH-018 Pentanoic Acid: 50 ng/mL JWH-073 Butanoic Acid: 25 ng/mL	CE	W089-P1G1
W55-S	KET (ketamine)	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL 300 ng/mL	CE	W055-S1G1 W055-S1G3001
W55-C	KET (ketamine)	Cassette	4.0mm	Urine	1000 ng/mL 300 ng/mL	CE	W055-C1G1 W055-C1G3001
W55-P	KET (ketamine)	Panel	4.0mm	Urine	1000 ng/mL 300 ng/mL		W055-P1G W055-P1G3001
W12-S	MDMA	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL 500 ng/mL	CE FDA	WW012-S1G10001 W012-S1G1
W12-C	MDMA	Cassette	4.0mm	Urine	1000 ng/mL 500 ng/mL	CE FDA	W012-C1G10001 W012-C1G1
W12-P	MDMA	Panel	4.0mm	Urine	1000 ng/mL 500 ng/mL	FDA CLIA	W012-P1G10001 W012-P1G1
W11-S	MET (Methamphetamine)	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL 500 ng/mL	CE FDA CE	W011-S1G1 W011-S1G5001
W11-C	MET (Methamphetamine)	Cassette	4.0mm	Urine	1000 ng/mL 500 ng/mL	CE FDA FDA CLIA	W011-C1G1 W011-C1G5001
W11-P	MET (Methamphetamine)	Panel	4.0mm	Urine	1000 ng/mL 500 ng/mL	FDA CLIA CE FDA CLIA	W011-P1G1 W011-P1G5001
W14-S	MOP (Morphine)	Strip	2.5/3.0/3.5/4.0mm	Urine	500 ng/mL 300 ng/mL 100 ng/mL	CE FDA	W014-S1G5001 W014-S1G1 W014-S1G1001
W14-C	MOP (Morphine)	Cassette	4.0mm	Urine	500 ng/mL 300 ng/mL 100 ng/mL	CE FDA	W014-C1G5001 W014-C1G1 W014-C1G1001
W14-P	MOP (Morphine)	Panel	4.0mm	Urine	500 ng/mL 300 ng/mL 100 ng/mL	FDA CLIA	W014-P1G5001 W014-P1G1 W014-P1G1001
W147-S	MC(Methcathinone)	Strip	4.0mm	Urine	1000 ng/mL		W147-S1G1
W147-C	MC(Methcathinone)	Cassette	4.0mm	Urine	1000 ng/mL		W147-C1G1
W147-P	MC(Methcathinone)	Panel	4.0mm	Urine	1000 ng/mL		W147-P1G1
W155-S	MQL(Methaqualone)	Strip	4.0mm	Urine	300 ng/mL		W155-S1G1
W155-C	MQL(Methaqualone)	Cassette	4.0mm	Urine	300 ng/mL		W155-C1G1
W155-P	MQL(Methaqualone)	Panel	4.0mm	Urine	300 ng/mL		W155-P1G1
W15-S	MTD (Methadone)	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL 200 ng/mL	CE FDA	W015-S1G1 W015-S1G2001
W15-C	MTD (Methadone)	Cassette	4.0mm	Urine	300 ng/mL 200 ng/mL	CE FDA	W015-C1G1 W015-C1G2001
W15-P	MTD (Methadone)	Panel	4.0mm	Urine	300 ng/mL 200 ng/mL	FDA CLIA FDA	W015-P1G1 W015-P1G2001
W16-S	OPI (Opiate)	Strip	2.5/3.0/3.5/4.0mm	Urine	2000 ng/mL 300 ng/mL	CE FDA	W016-S1G1 W016-S1G3001
W16-C	OPI (Opiate)	Cassette	4.0mm	Urine	2000 ng/mL 300 ng/mL	CE FDA	W016-C1G1 W016-C1G3001
W16-P	OPI (Opiate)	Panel	4.0mm	Urine	2000 ng/mL 300 ng/mL	FDA CLIA	W016-P1G1 W016-P1G3001
W21-S	OXY (Oxycodone)	Strip	2.5/3.0/3.5/4.0mm	Urine	100 ng/mL	CE FDA	W021-S1G1
W21-C	OXY (Oxycodone)	Cassette	4.0mm	Urine	100 ng/mL	CE	W021-C1G1
W21-P	OXY (Oxycodone)	Panel	4.0mm	Urine	100 ng/mL	FDA CLIA	W021-P1G1

## Drug of Abuse Tests (Urine)

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W17-S	PCP (Phencyclidine)	Strip	2.5/3.0/3.5/4.0mm	Urine	25 ng/mL	CE FDA	W017-S1G1
W17-C	PCP (Phencyclidine)	Cassette	4.0mm	Urine	25 ng/mL	CE FDA	W017-C1G1
W17-P	PCP (Phencyclidine)	Panel	4.0mm	Urine	25 ng/mL	FDA CLIA	W017-P1G1
W57-S	PPX (Propoxyphene)	Strip	2.5/3.0/3.5/4.0mm	Urine	300 ng/mL	CE FDA	W057-S1G1
W57-C	PPX (Propoxyphene)	Cassette	4.0mm	Urine	300 ng/mL	CE	W057-C1G1
W57-P	PPX (Propoxyphene)	Panel	4.0mm	Urine	300 ng/mL	FDA CLIA	W057-P1G1
W18-S	TCA (Tricyclic Antidepressants)	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL	CE FDA	W018-S1G1
W18-C	TCA (Tricyclic Antidepressants)	Cassette	4.0mm	Urine	1000 ng/mL	CE FDA	W018-C1G1
W18-P	TCA (Tricyclic Antidepressants)	Panel	4.0mm	Urine	1000 ng/mL	FDA CLIA	W018-P1G1
W19-S	THC (Marijuana)	Strip	2.5/3.0/3.5/4.0mm	Urine	50 ng/mL	CE FDA	W019-S1G1
W19-S	THC (Marijuana)	Strip	2.5/3.0/3.5/4.0mm	Urine	50 ng/mL	CE FDA	W019-S1G1
					40 ng/mL		W019-S1G401
					25 ng/mL	CE	W019-S1G251
					50 ng/mL	CE FDA	W019-C1G1
W19-C	THC (Marijuana)	Cassette	4.0mm	Urine	40 ng/mL		W019-C1G401
W19-P	THC (Marijuana)	Panel	4.0mm	Urine	25 ng/mL	CE	W019-C1G251
					50 ng/mL	FDA CLIA	W019-P1G1
					40 ng/mL	FDA	W019-P1G401
					25 ng/mL	CE	W019-P1G251
W086-S	TRA (Tramadol)	Strip	2.5/3.0/3.5/4.0mm	Urine	1000 ng/mL	CE	W086-S1G1
W086-C	TRA (Tramadol)	Cassette	4.0mm	Urine	1000 ng/mL	CE	W086-C1G1
W086-P	TRA (Tramadol)	Panel	4.0mm	Urine	1000 ng/mL	CE	W086-P1G1
W086-S	TRA (Tramadol)	Strip	2.5/3.0/3.5/4.0mm	Urine	200 ng/mL		W086-S1G2001
W086-C	TRA (Tramadol)	Cassette	4.0mm	Urine	200 ng/mL		W086-C1G2001
W086-P	TRA (Tramadol)	Panel	4.0mm	Urine	200 ng/mL		W086-P1G2001
W086-S	TRA (Tramadol)	Strip	2.5/3.0/3.5/4.0mm	Urine	100 ng/mL		W086-S1G1001
W086-C	TRA (Tramadol)	Cassette	4.0mm	Urine	100 ng/mL		W086-C1G1001
W086-P	TRA (Tramadol)	Panel	4.0mm	Urine	100 ng/mL		W086-P1G1001

## Drug of Abuse (Oral fluid)

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W6506	Oral Fluid Multi-Drug 6 Test	Panel	/	Oral Fluid	Variable	/	W606-P91
W602~610-CU6	Multi-Drug Oral Fluid 2~10	T-Cube	4.0mm	Oral Fluid	Variable	/	W602~610-CU69G1
W53-S	Alcohol saliva Test	Strip	3.5/4.0mm	Saliva	Custom	CE	W402-S9G1

## Other Rapid Tests

Cat. No.	Test Item	Format	Width	Specimen	Sensitivity	Qualification	Product Code
W5410-S	Urinalysis Reagents Strip (1~10 Parameter)	Strip	5.0 mm	Urine	/	CE	/

## Quantitative Detection Family

- **Fineware™ Platform**



**Fineware™ Automatic (FS-302)**



**Fineware™ FIA Meter III Plus (FS-205)**



**Fineware™ FIA Meter Plus (FS-113)**



**Fineware™ FIA Meter (FS-112)**



## Immunofluorescence Quantitative Test System FS-112/FS-113/FS-205

**Finicare™ FIA Meter serie** is a fluorescence immunochromatographic analysing system which can help diagnose conditions such as infection, diabetes, cardiovascular diseases, renal injury and cancers, etc.

The Finicare™ platform provides reliable and quantitative results of various kinds of analytes in human blood or urine within several minutes.

**Application:** Laboratory, ER, Cardiology, ICU, Respiratory, Pediatrics, etc.

Cat. No.	Test Item	Specimen Type	Sample Volume	Reaction Time	Measuring Range	Qualification	Product Code
W210	PCT	S/P/WB	50/75µL	15 min	0.1-100 ng/mL	CE	W210-C4PM
W201	CRP	S/P/WB	5/8.5µL	3 min	0.5-200 mg/L	CE	W201-C4PM
W218	CRP/PCT	S/P/WB	75µL	15 min	CRP: 0.5-150 mg/L PCT: 0.1-100 ng/mL	CE	W218-C4PM
W221	SAA	S/P/WB	10µL	15 min	1.0-300 mg/L	CE	W221-C4PM
W211	D-Dimer	P/WB	75µL	5 min	0.1-10 mg/L	CE	W211-C0PM
W202	NT-proBNP	S/P/WB	75µL	15 min	18-35000 pg/mL	CE	W202-C4PM
W203	cTn I	S/P/WB	75µL	15 min	0.1-50 ng/ml	CE	W203-C4PM
W204	Myo	S/P/WB	75µL	15 min	2.0-400 ng/mL	CE	W204-C4PM
W205	CK-MB	S/P/WB	75µL	15 min	0.30-100 ng/mL	CE	W205-C4PM
W217	H-FABP	S/P/WB	75µL	15 min	1-120 ng/mL	CE	W217-C4PM
W216	cTn I/CK-MB/Myo	S/P/WB	75µL	15 min	Same with single item	CE	W216-C4PM
W222	BNP	S/P/WB	75µL	15 min	5-5000 pg/mL	CE	W222-C0PM
W223	cTn I/ NT-proBNP	S/P/WB	75µL	15 min	Same with single item	CE	W223-C4PM
W208	AFP	S/P/WB	75µL	15 min	5-400 ng/mL	CE	W208-C8PM
W209	PSA	S/P/WB	75µL	15 min	2-100 ng/mL	CE <sub>0123</sub>	W209-C8PM
W230	FPSA	S/P/WB	75µL	15 min	0.2-30 ng/mL	CE <sub>0123</sub>	W230-C4PM
W226	CEA	S/P/WB	75µL	15 min	1-500 ng/mL	CE	W226-C4PM
W207	HbA1c	WB	/	5 min	4.0-14.5%	CE  	W207-C7PM
W206	MAU	Urine	75µL	3 min	5-300 mg/L	CE	W206-C1PM
W219	Cys C	S/P/WB	10µL	5 min	0.2-10 mg/L	CE	W219-C4PM
W228	NGAL	Urine	75µL	15 min	10-1500 ng/mL	CE	W228-C1PM
W229	β2-MG	S/P/WB	10µL	10 min	0.3-20 mg/L	CE	W229-C4PM
W225	β-hCG	S/P/WB	20µL	15 min	2-200000 mIU/mL	CE	W225-C4PM
W231	T3	S/P/WB	75µL	15 min	0.61-9.22 nmol/L	CE	W231-C4PM
W232	T4	S/P/WB	75µL	15 min	12.87-300 nmol/L	CE	W232-C4PM
W220	TSH	S/P/WB	75µL	15 min	0.1-100 mIU/L	CE	W220-C4PM
W244	LH	S/P/WB	75µL	15 min	1-100 mIU/L	CE	W244-C4PM
W245	FSH	S/P/WB	75µL	15 min	1-100 mIU/L	CE	W245-C4PM
W233	Prog	S/P/WB	75µL	15 min	1.5-60 ng/mL	CE	W233-C4PM
W246	PRL	S/P/WB	75µL	15 min	1-200 ng/mL	CE	W246-C4PM
W241	Vitamin D	S/P	75µL	15 min	5-100 ng/mL	CE	W241-C4PM



**\* Ongoing: Testosterone, Cortisol, Lp-PLA2**

## Blood Gas Analyzer BGA-101



pH, pCO<sub>2</sub>, pO<sub>2</sub>, K<sup>+</sup>, Na<sup>+</sup>, Ca<sup>++</sup>, Cl<sup>-</sup>, Hct, Glu\*, Lac\*

Calculation Parameters: cH<sup>+</sup>, cH<sup>+</sup>(T), pH(T), pCO<sub>2</sub>(T), pO<sub>2</sub>(T), HCO<sub>3</sub><sup>-</sup>atd, HCO<sub>3</sub><sup>-</sup>std, BB(B), BE(B), BE(ecf), ct CO<sub>2</sub>, Ca<sup>++</sup>(7.4), AnGap, tHb(est), sO<sub>2</sub>(est), pO<sub>2</sub>(A-a), pO<sub>2</sub>(A-a)(T), pO<sub>2</sub>(a/A), pO<sub>2</sub>(a/A)(T), RI, RI(T), pO<sub>2</sub>/FI O<sub>2</sub>, pO<sub>2</sub>(T)/FI O<sub>2</sub>

### Specifications:

- Sample Type: Whole Blood
- Sample Volume: 80 µL
- Reading Time: 30 s
- Suitable for Syringe and Capillary
- Memory:>50,000
- Good Correlation to Reference Method: R<sup>2</sup>>0.95



## Test Packages

Test Item	Cat No.	W459	W460	W461	W462	W463	W464	W465	W466 *
pH		•			•	•	•	•	•
pCO <sub>2</sub>		•			•	•	•	•	•
pO <sub>2</sub>		•			•	•	•	•	•
K <sup>+</sup>			•	•	•	•	•	•	•
Na <sup>+</sup>			•	•	•	•	•	•	•
Ca <sup>++</sup>				•			•	•	•
Cl <sup>-</sup>			•	•	•	•		•	•
Hct						•	•	•	•
Glu*									•
Lac*									•

\* Ongoing

## Optical Coagulation Analyzer OCG-102



Cat. No.	Test Item	Specimen	Specification	Qualification	Product Code
OCG-102	Optical Coagulation Analyzer	/	1 Meter	CE	/
W459-W466	PT/APTT/TT/FIB/ACT	Citrated Venous Whole Blood and Capillary Blood (PT/INR only)	24 T/Kit	CE	/



PT/INR, APTT, TT, FIB, ACT

### Specifications:


- **Sample Type:** Citrated Venous Whole Blood and Capillary Blood (PT/INR Only)
- **Sample Volume:** 20 µL
- **Time to Result:** ≤5 minutes
- **Precision:** CV≤5%
- **Store at room temperature and valid for 18 months**



## Blood Glucose Monitoring System

Cat. No.	Test Item	Specimen	Specification	Qualification	Product Code
WM801W02	Blood Glucose Monitoring System	/	1 Meter	CE 0123	/
W301	Blood Glucose Test Strip	Capillary Whole blood	50 T/Kit	CE 0123	W301-S7G


### • Glucose Meter



# Wondfo®

## OUR VISION

Provide professional products and services of rapid diagnosis and chronic disease management; Pursue better and convenient user experience; Promote high-standard life and health quality; Fulfill shared dream of our staff, customers and partners.

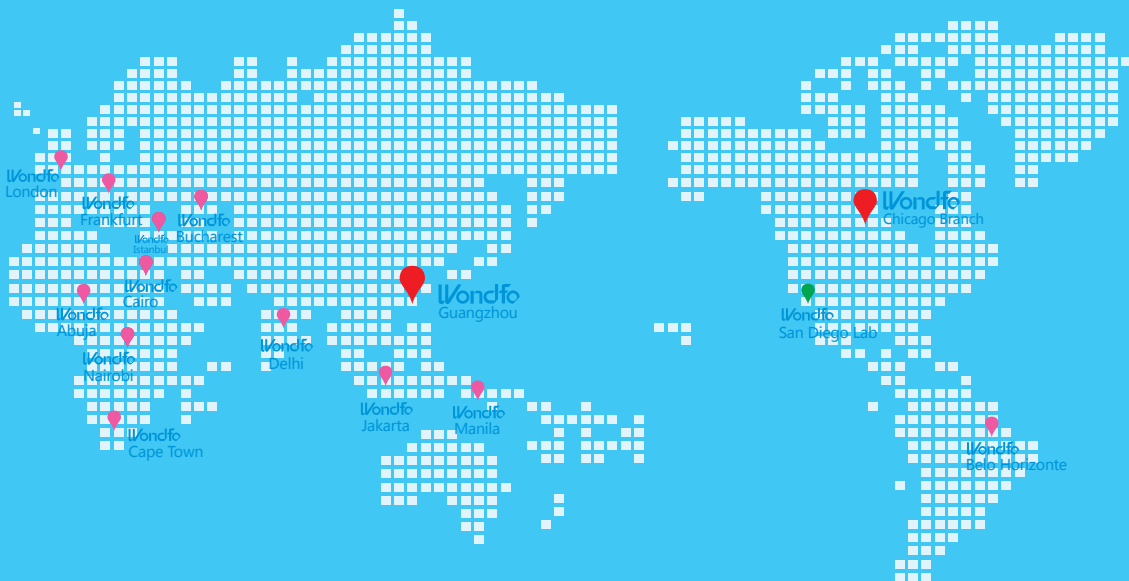

**1,500+** Employees

**200+** R&D Staffs

**1** Overseas Lab

**1** Branch

**10+** Overseas Offices

WONDFO BIOTECH  
WeAreWorkingForYourHealth

Wondfo®

**Guangzhou Wondfo Biotech Co., Ltd.**

No. 8 Lizhishan Road, Science City, Luogang District,  
510663, Guangzhou, P.R. China

Tel: +86-20-32296083  
Fax: +86-20-32296063  
E-mail: [sales@wondfo.com.cn](mailto:sales@wondfo.com.cn)  
Website: [www.wondfo.com.cn](http://www.wondfo.com.cn)

Customers Service Center:  
Tel: +86-20-32296083  
Fax: +86-20-32296063  
E-mail: [customerservice@wondfo.com.cn](mailto:customerservice@wondfo.com.cn)